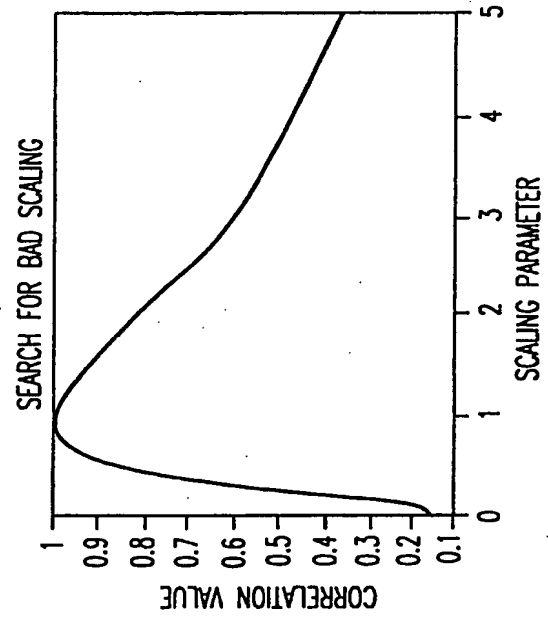
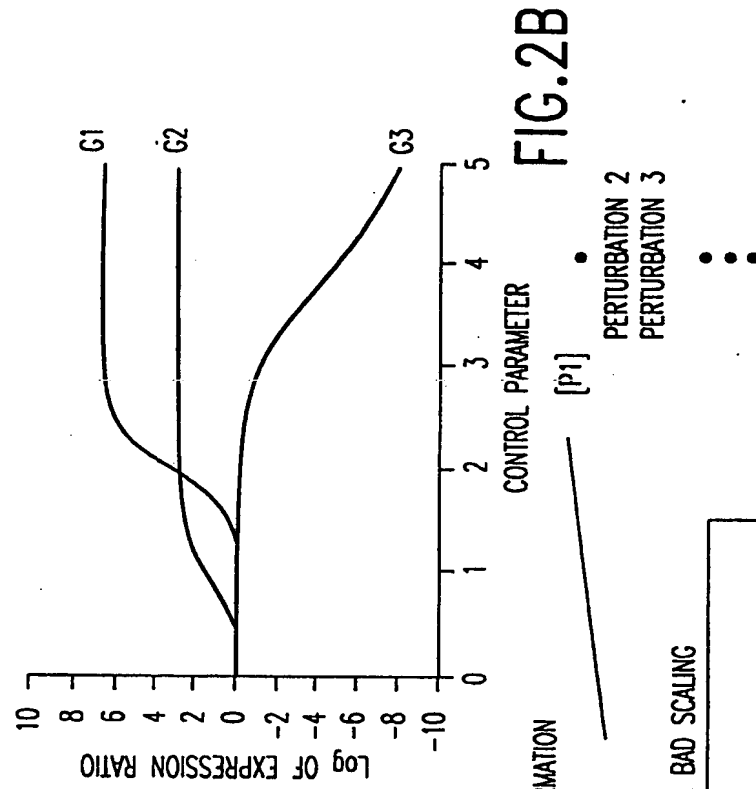
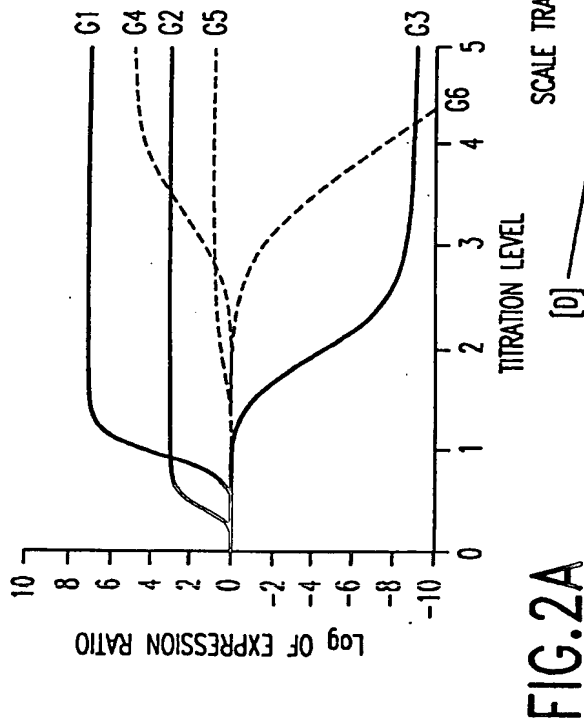


FIG. 1

T03040" 2322860



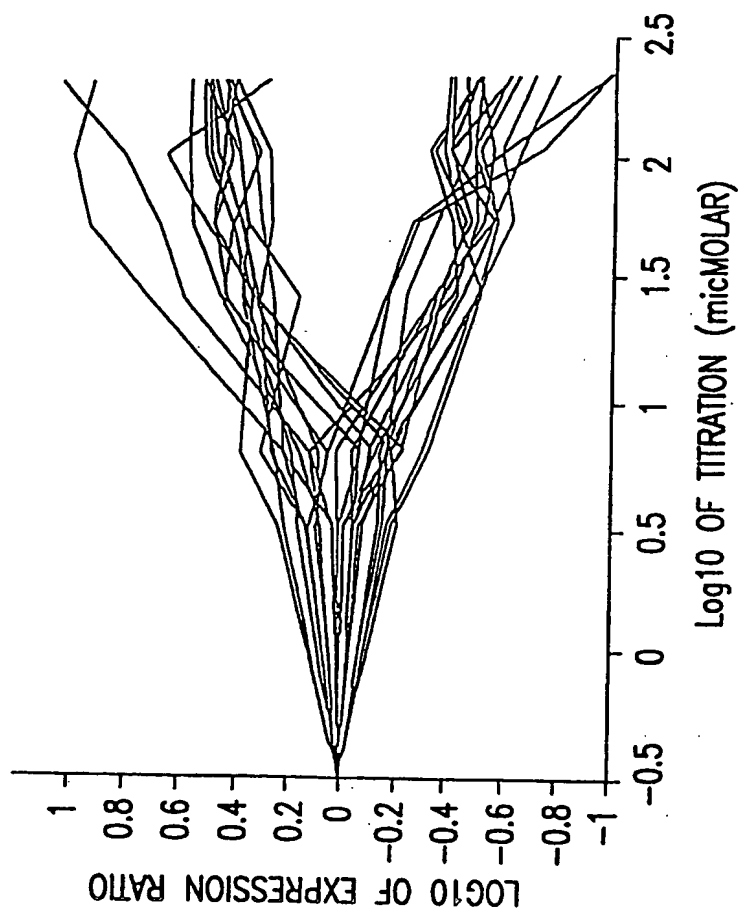


FIG.3

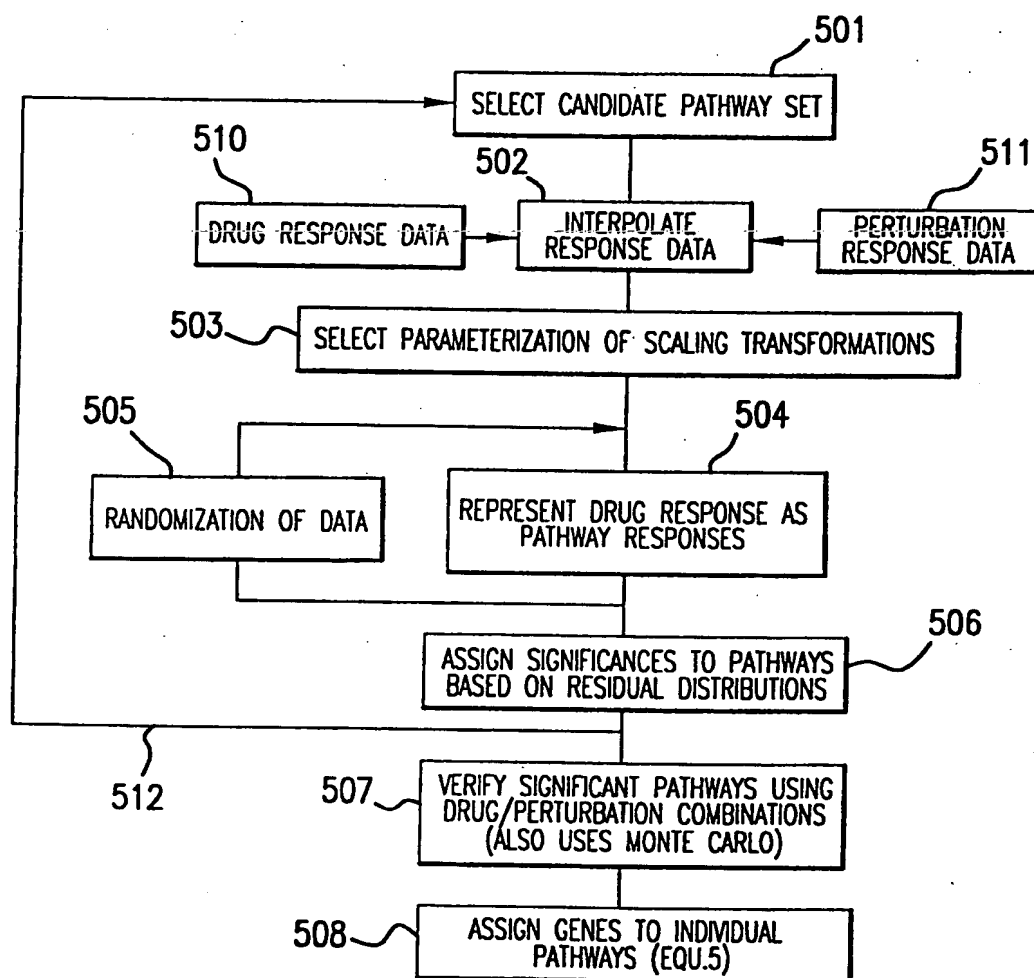


FIG.5



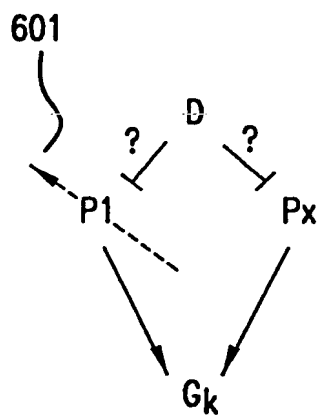


FIG.6

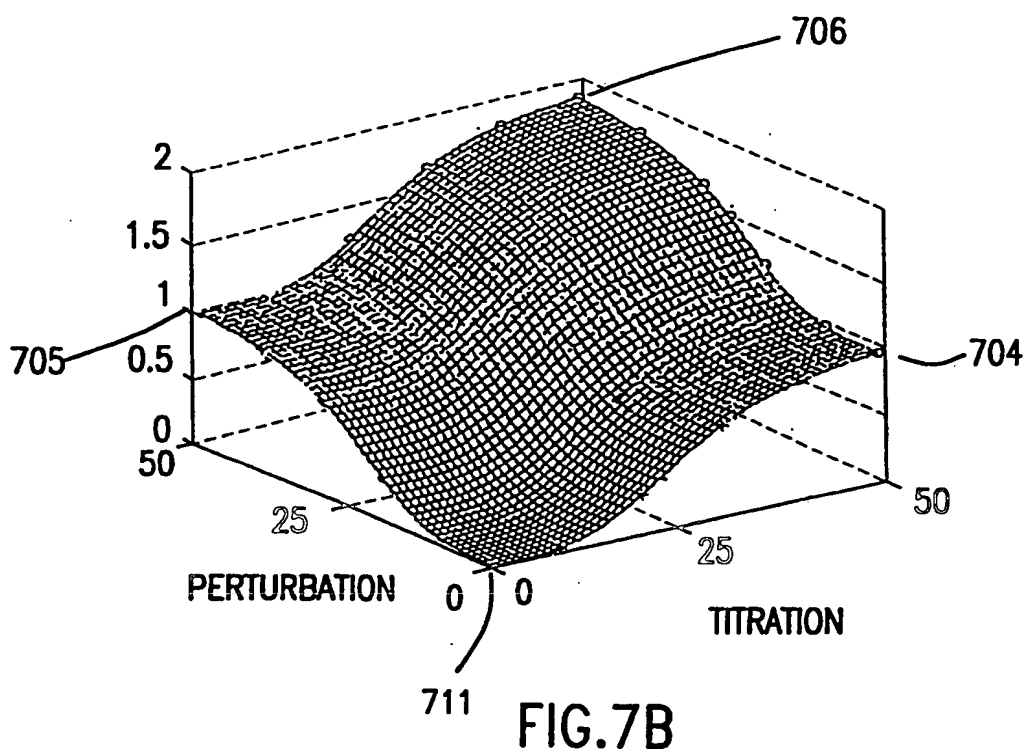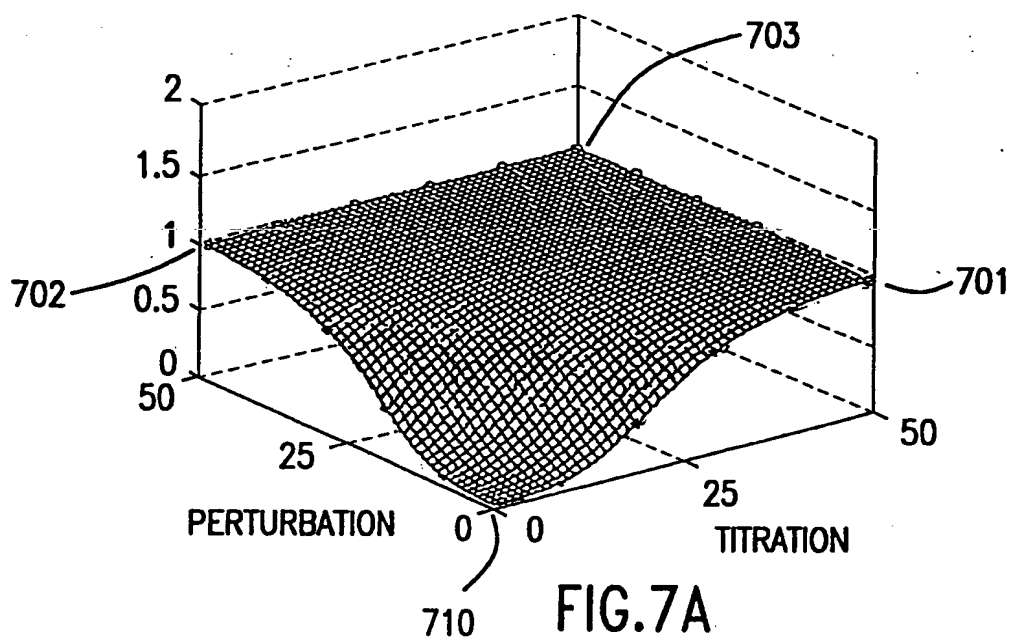

FK506 TITRATION SERIES

LOG₁₀ THRESHOLD: 0.30

Pvalue: 0.30

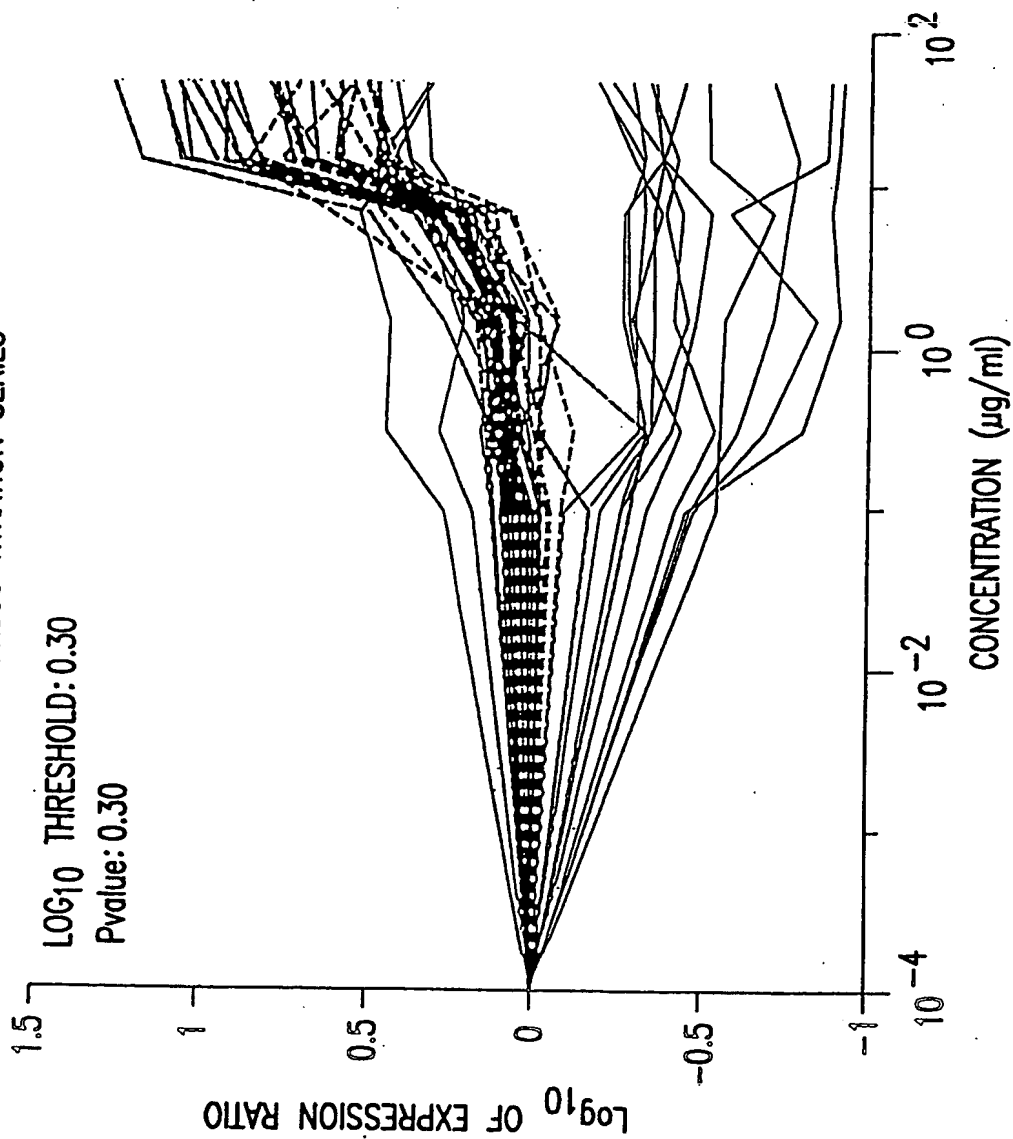


FIG.8A

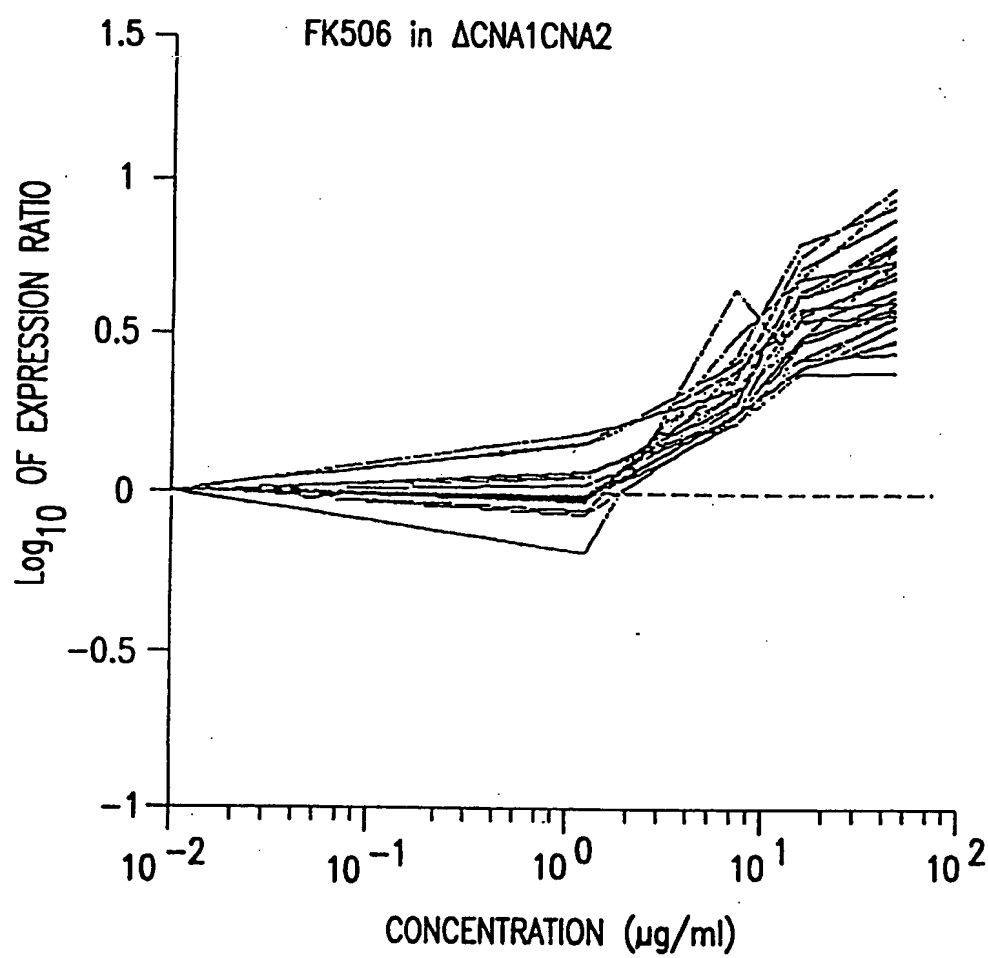


FIG.8B

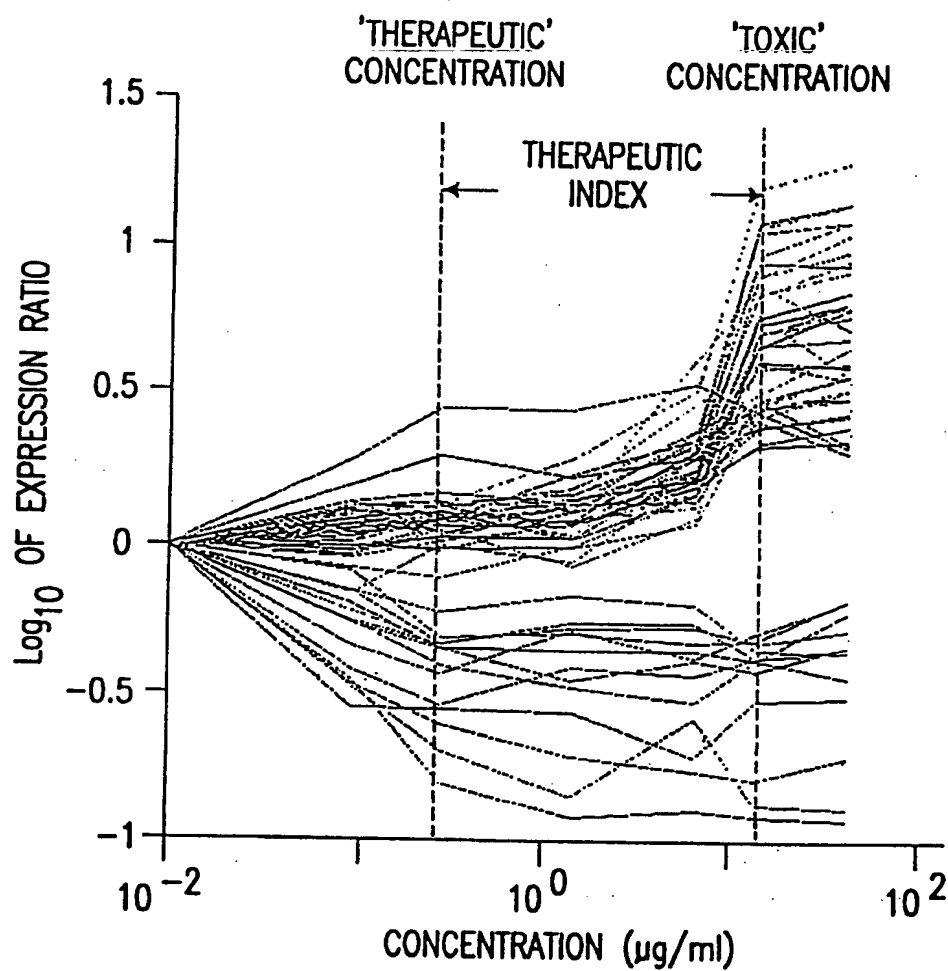


FIG.8C

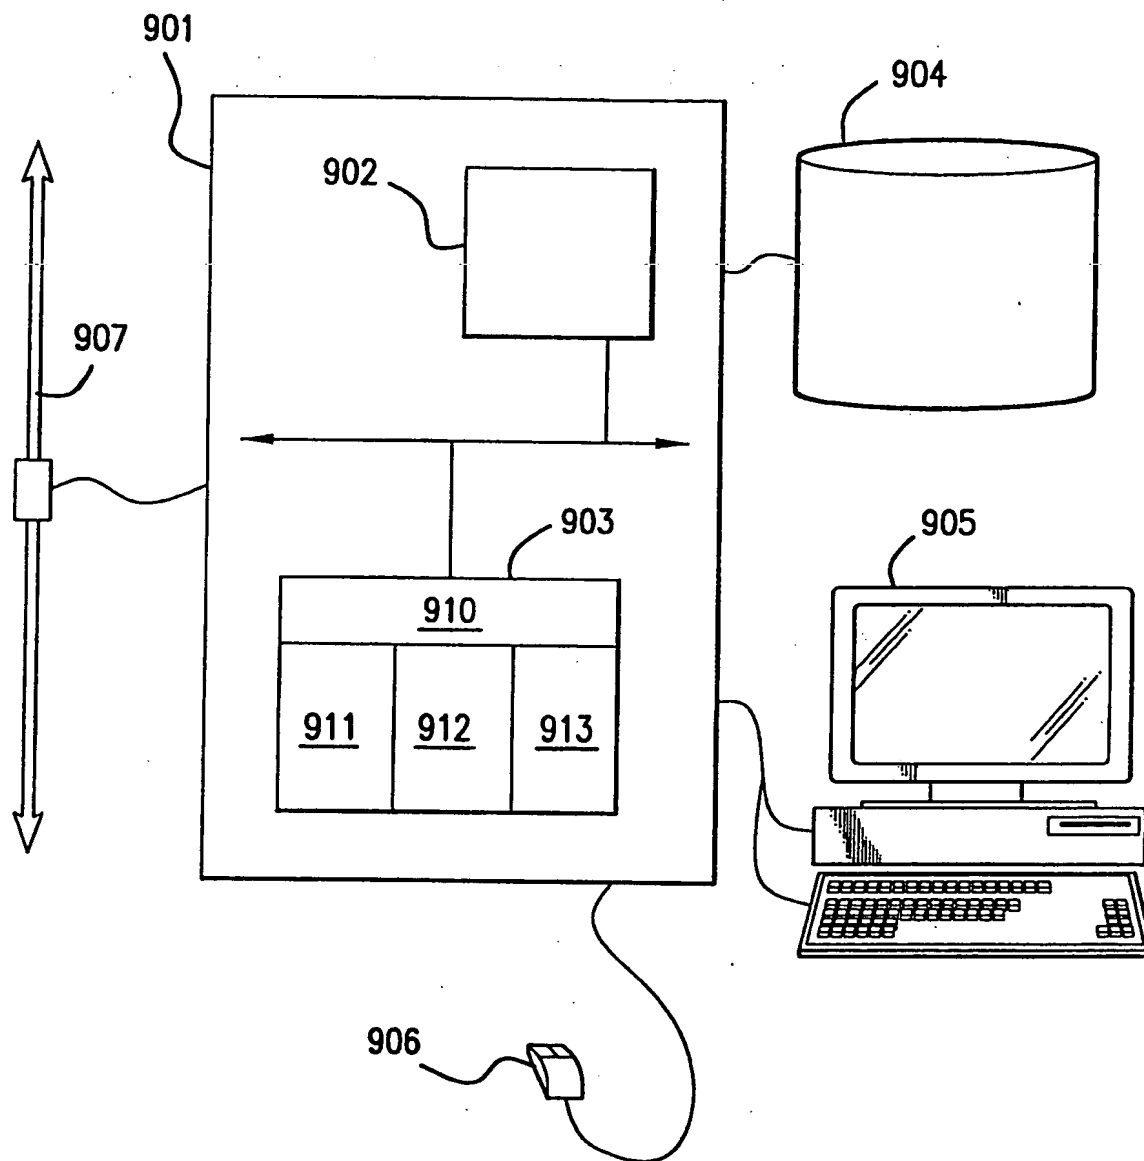


FIG. 9